

Alcotest 7110 Calibration Record

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0171
Location: NJSP SAYREVILLE
Calibration File No.: 00006 Calib. Date: 01/05/2009 Calib. No.: 00004
Certification File No.: 00000 Cert. Date: --/--/---- Cert. No.: 00000
Linearity File No.: 00000 Lin. Date: --/--/---- Lin. No.: 00000
Solution File No.: 00005 Soln. Date: 12/03/2008 Soln. No.: 00001
Sequential File No.: 00006 File Date: 01/05/2009


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWB S3-0062
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 0702

Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.
Signature: TAR. I Thomas J. Snyder #5792 Badge No.: 5792
Date: 01/05/2009

*Black Key Temperature Probe Serial# DDUN P2-229 JAS

*Ertco-Hart Digital Temperature Measuring System Serial# A29881 JAS

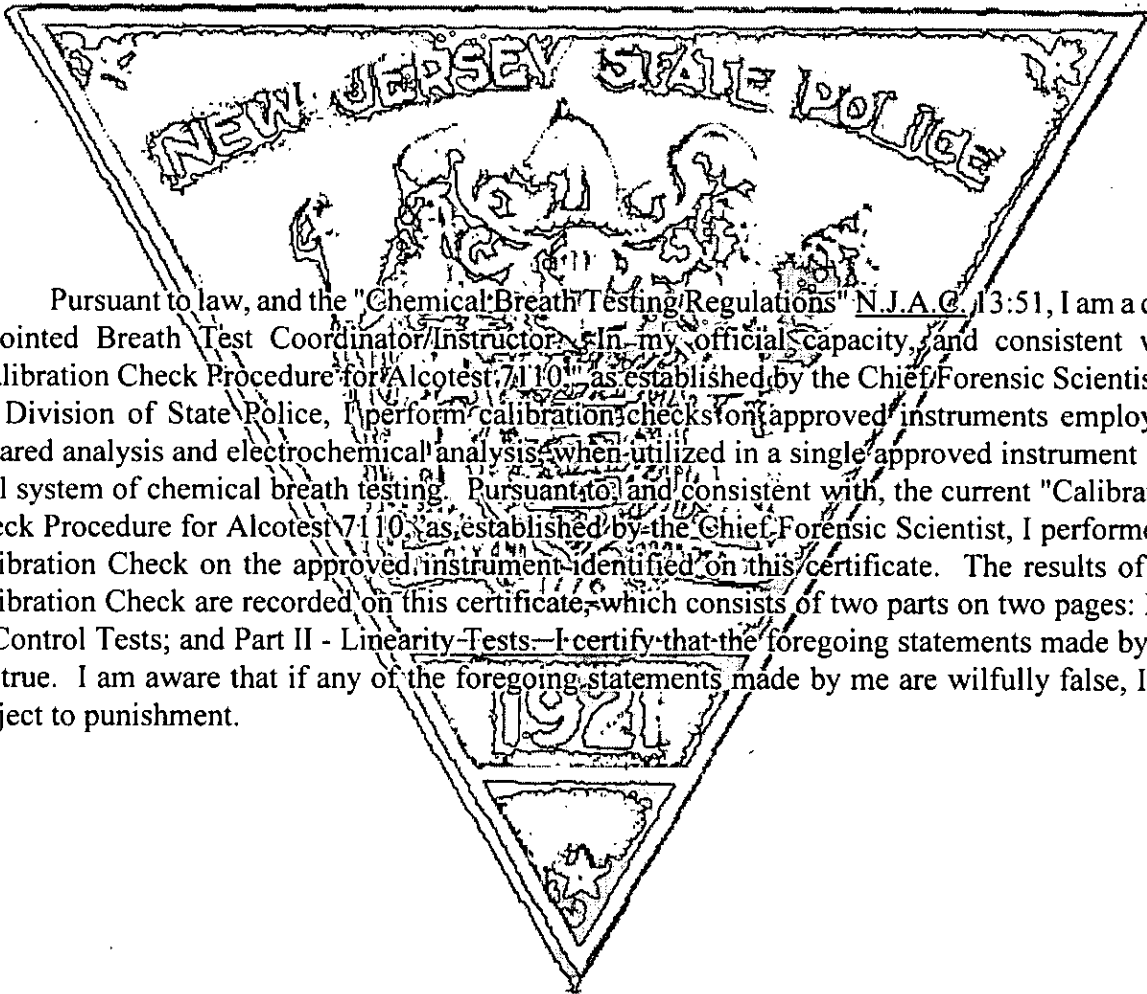

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0171
Location: NJSP SAYREVILLE
Calibration File No.: 00006 Calib. Date: 01/05/2009 Calib. No.: 00004
Certification File No.: 00007 Cert. Date: 01/05/2009 Cert. No.: 00001
Linearity File No.: 00000 Lin. Date: --/--/---- Lin. No.: 00000
Solution File No.: 00005 Soln. Date: 12/03/2008 Soln. No.: 00001
Sequential File No.: 00007 File Date: 01/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWB S3-0062
Control Solution %: 0.100% Expires: 07/02/2010
Solution Control Lot: 08G056 Bottle No.: 0702

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:07S		
Control 1 EC	0.099%	11:08S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:08S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08S		
Control 2 EC	0.099%	11:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:09S		
Control 3 EC	0.099%	11:10S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:10S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:11S		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

Signature: *TH. J. Snyder*

First Name: THOMAS

Badge No.: 5792

Date: 01/05/2009

MI: J.

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWA-0171
Location: NJSP SAYREVILLE
Calibration File No.: 00006 Calib. Date: 01/05/2009 Calib. No.: 00004
Certification File No.: 00007 Cert. Date: 01/05/2009 Cert. No.: 00001
Linearity File No.: 00008 Lin. Date: 01/05/2009 Lin. No.: 00001
Solution File No.: 00005 Soln. Date: 12/03/2008 Soln. No.: 00001
Sequential File No.: 00008 File Date: 01/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003
Control Solution %: 0.040% Expires: 06/26/2010
Solution Control Lot: 08F054 Bottle No.: 0153

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184
Control Solution %: 0.080% Expires: 06/28/2010
Solution Control Lot: 08F055 Bottle No.: 0347

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009
Control Solution %: 0.160% Expires: 07/07/2010
Solution Control Lot: 08G057 Bottle No.: 1398

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:53S		
Control 1 EC	0.040%	11:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.042%	11:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		
Control 2 EC	0.040%	11:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	11:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 3 EC	0.078%	11:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.077%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58S		
Control 4 EC	0.079%	11:59S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	11:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:00S		
Control 5 EC	0.157%	12:01S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.155%	12:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02S		
Control 6 EC	0.158%	12:03S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.158%	12:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 01/05/2009

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0171
Location:	NJSP SAYREVILLE	
Calibration File No.:	00107	Calib. Date: 07/02/2009
Certification File No.:	00108	Calib. No.: 00005
Linearity File No.:	00008	Cert. Date: 07/02/2009
Solution File No.:	00097	Cert. No.: 00002
Sequential File No.:	00108	Lin. Date: 01/05/2009
		Lin. No.: 00001
		Soln. Date: 06/18/2009
		Soln. No.: 00010
		File Date: 07/02/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWB S3-0062
Solution Control Lot:	08G056	Expires: 07/02/2010
		Bottle No.: 0393

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:45D		
Control 1 EC	0.099%	08:45D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:45D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:46D		
Control 2 EC	0.099%	08:46D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:46D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47D		
Control 3 EC	0.099%	08:48D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:48D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:48D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature:

T.P.R. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 07/02/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0171
Location:	NJSP SAYREVILLE	
Calibration File No.:	00107	Calib. Date: 07/02/2009
Certification File No.:	00108	Calib. No.: 00005
Linearity File No.:	00109	Cert. Date: 07/02/2009
Solution File No.:	00097	Cert. No.: 00002
Sequential File No.:	00109	Lin. Date: 07/02/2009
		Lin. No.: 00002
		Soln. Date: 06/18/2009
		Soln. No.: 00010
		File Date: 07/02/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.040%	Serial No.: DDRK S3-0003
Solution Control Lot:	08F054	Expires: 06/26/2010
		Bottle No.: 1228
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.080%	Serial No.: DDXD S3-0184
Solution Control Lot:	08F055	Expires: 06/28/2010
		Bottle No.: 0801
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.160%	Serial No.: DDSC S3-0009
Solution Control Lot:	08G057	Expires: 07/07/2010
		Bottle No.: 0414

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:29D		
Control 1 EC	0.041%	09:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32D		
Control 2 EC	0.040%	09:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		
Control 3 EC	0.080%	09:34D	33.8°C	*** TEST PASSED ***
Control 3 IR	0.079%	09:34D	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36D		
Control 4 EC	0.079%	09:36D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	09:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38D		
Control 5 EC	0.158%	09:38D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	09:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40D		
Control 6 EC	0.157%	09:40D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	09:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: *TPR. I Thomas J. Snyder #5792*

Badge No.: 5792

Date: 07/02/2009

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0171
Location:	NJSP HOLMDEL	
Calibration File No.:	00227	Calib. Date: 12/30/2009
Certification File No.:	00228	Calib. No.: 00006
Linearity File No.:	00109	Cert. Date: 12/30/2009
Solution File No.:	00221	Cert. No.: 00003
Sequential File No.:	00228	Lin. Date: 07/02/2009
		Lin. No.: 00002
		Soln. Date: 12/17/2009
		Soln. No.: 00021
		File Date: 12/30/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWB S3-0065
Solution Control Lot:	09D065	Expires: 04/22/2011
		Bottle No.: 0467


Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:23S		
Control 1 EC	0.100%	09:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:24S		
Control 2 EC	0.098%	09:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25S		
Control 3 EC	0.098%	09:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27S		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.
 Signature: *TPR. I Thomas J. Snyder #5792* Badge No.: 5792 Date: 12/30/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

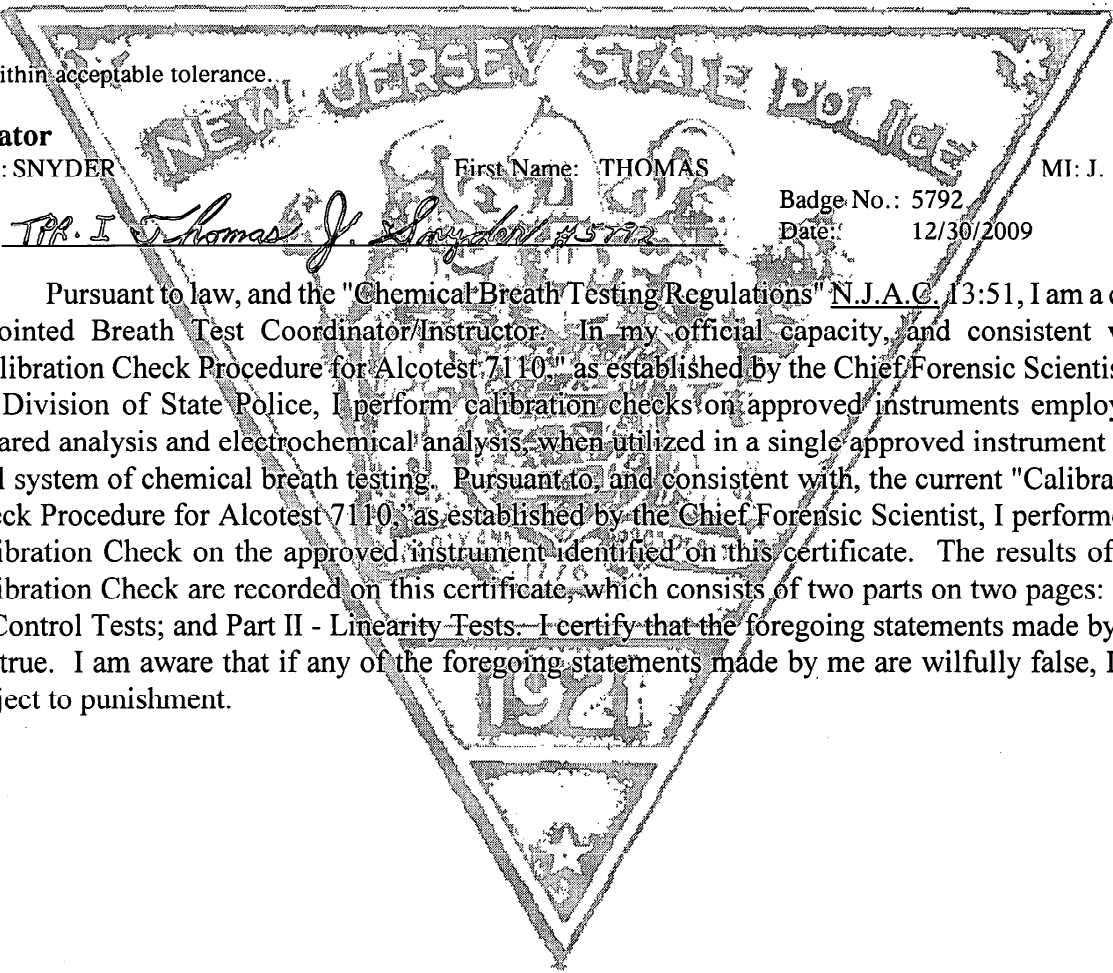

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWA-0171
Location:	NJSP HOLMDEL	
Calibration File No.:	00227	Calib. Date: 12/30/2009
Certification File No.:	00228	Calib. No.: 00006
Linearity File No.:	00229	Cert. Date: 12/30/2009
Solution File No.:	00221	Cert. No.: 00003
Sequential File No.:	00229	Lin. Date: 12/30/2009
		Lin. No.: 00003
		Soln. Date: 12/17/2009
		Soln. No.: 00021
		File Date: 12/30/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.040%	Serial No.: DDRK S3-0003
Solution Control Lot:	08F054	Expires: 06/26/2010
		Bottle No.: 0853
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.080%	Serial No.: DDXD S3-0184
Solution Control Lot:	08F055	Expires: 06/28/2010
		Bottle No.: 0853
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.160%	Serial No.: DDSC S3-0009
Solution Control Lot:	08G057	Expires: 07/07/2010
		Bottle No.: 0853

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:43S		
Control 1 EC	0.042%	09:43S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:43S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45S		
Control 2 EC	0.041%	09:46S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.042%	09:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 3 EC	0.083%	09:48S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:48S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50S		
Control 4 EC	0.080%	09:51S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52S		
Control 5 EC	0.159%	09:53S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	09:53S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54S		
Control 6 EC	0.159%	09:55S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	09:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 12/30/2009

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0171
Location:	NJSP HOLMDEL		
Calibration File No.:	00333	Calib. Date:	06/30/2010
Certification File No.:	00334	Cert. Date:	06/30/2010
Linearity File No.:	00229	Lin. Date:	12/30/2009
Solution File No.:	00331	Soln. Date:	06/29/2010
Sequential File No.:	00334	File Date:	06/30/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWB S3-0065
Solution Control Lot:	09D065	Expires:	04/22/2011
		Bottle No.:	0711

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:02D		
Control 1 EC	0.099%	09:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04D		
Control 2 EC	0.099%	09:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05D		
Control 3 EC	0.099%	09:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:06D		

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

Signature: *T.P. II*


First Name: T.P. II

Badge No.: 5925

Date: 06/30/2010

MI: WJ

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized as a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

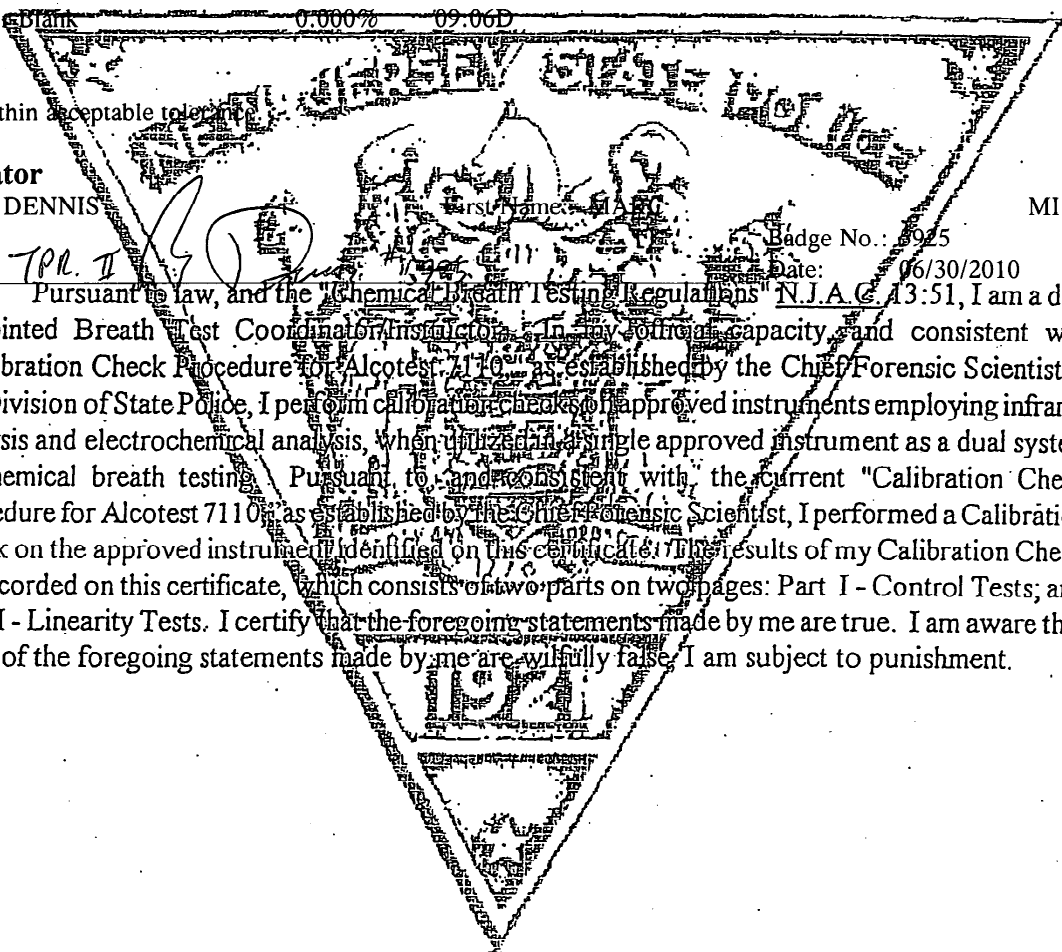

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWA-0171
Location:	NJSP HOLMDEL		
Calibration File No.:	00333	Calib. Date:	06/30/2010
Certification File No.:	00334	Cert. Date:	06/30/2010
Linearity File No.:	00335	Lin. Date:	06/30/2010
Solution File No.:	00331	Soln. Date:	06/29/2010
Sequential File No.:	00335	File Date:	06/30/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDXD S3-0186
Solution Control Lot:	10A073	Expires:	01/12/2012
		Bottle No.:	0347
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDXD S3-0188
Solution Control Lot:	10A074	Expires:	01/15/2012
		Bottle No.:	0475
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDXD S3-0191
Solution Control Lot:	10A075	Expires:	01/21/2012
		Bottle No.:	1021

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:26D		
Control 1 EC	0.042%	09:27D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	09:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		
Control 2 EC	0.041%	09:29D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	09:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:30D		
Control 3 EC	0.082%	09:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32D		
Control 4 EC	0.080%	09:33D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		
Control 5 EC	0.162%	09:35D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.164%	09:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:36D		
Control 6 EC	0.160%	09:37D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.162%	09:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:38D		

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: TPR. II [Signature] # 5925

Badge No.: 5925

Date: 06/30/2010