

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWC-0005  
Location: N.J.S.P. - NEWARK BAY  
Calibration File No.: 00007 Calib. Date: 11/17/2008 Calib. No.: 00002  
Certification File No.: 00008 Cert. Date: 11/17/2008 Cert. No.: 00001  
Linearity File No.: 00009 Lin. Date: 11/17/2008 Lin. No.: 00001  
Solution File No.: 00010 Soln. Date: 11/17/2008 Soln. No.: 00002  
Sequential File No.: 00010 File Date: 11/17/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0183  
Control Solution %: 0.100% Expires: 03/07/2010  
Solution Control Lot: 08C051 Bottle No.: 0950

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:29S		
Control 1 EC	0.101%	12:30S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:30S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30S		
Control 2 EC	0.099%	12:31S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:31S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32S		
Control 3 EC	0.099%	12:32S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:32S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


TEMPERATURE PROBE SERIAL # DDXAP2-040 (RMD)

### Changed By:

Last Name: DEMLER

First Name: ROBERT

MI: M.

Signature: 

Badge No.: 6073

Date: 11/17/2008

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0005
Location:	N.J.S.P. - NEWARK BAY		
Calibration File No.:	00007	Calib. Date:	11/17/2008
Certification File No.:	00008	Cert. No.:	00002
Linearity File No.:	00009	Cert. Date:	11/17/2008
Solution File No.:	00011	Lin. Date:	11/17/2008
Sequential File No.:	00011	Soln. Date:	11/23/2008
		Soln. No.:	00003
		File Date:	11/23/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXD S3-0183
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0927

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:11S		
Control 1 EC	0.097%	07:11S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	07:11S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:12S		
Control 2 EC	0.096%	07:13S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:13S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:13S		
Control 3 EC	0.098%	07:14S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	07:14S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNEZLER      First Name: EDWARD      MI: J

Signature: *TPR. Edward J. Schnezler # 5515*

Badge No.: 5515  
Date: 11/23/2008

# Calibrating Unit New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C  
 Location: N.J.S.P. - NEWARK BAY  
 Serial No.: ARWC-0005  
 Calibration File No.: 00007      Calib. Date: 11/17/2008      Calib. No.: 00002  
 Certification File No.: 00008      Cert. Date: 11/17/2008      Cert. No.: 00001  
 Linearity File No.: 00009      Lin. Date: 11/17/2008      Lin. No.: 00001  
 Solution File No.: 00012      Soln. Date: 12/30/2008      Soln. No.: 00004  
 Sequential File No.: 00012      File Date: 12/30/2008

Calibrating Unit: WET      Model No.: CU-34      Serial No.: DDXD S3-0183  
 Control Solution %: 0.100%      Expires: 03/07/2010  
 Solution Control Lot: 08C051      Bottle No.: 0933

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:31S		
Control 1 EC	0.102%	23:32S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.102%	23:32S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:32S		
Control 2 EC	0.100%	23:33S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.102%	23:33S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:34S		
Control 3 EC	0.100%	23:35S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:35S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNEZLER      First Name: EDWARD      MI: J

Signature: *TRIE J. Schnezler #5515*      Badge No.: 5515  
 Date: 12/30/2008

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0005
Location:	N.J.S.P. - NEWARK BAY		
Calibration File No.:	00007	Calib. Date:	11/17/2008
Certification File No.:	00008	Cert. No.:	00002
Linearity File No.:	00009	Cert. Date:	11/17/2008
Solution File No.:	00013	Lin. Date:	11/17/2008
Sequential File No.:	00013	Lin. No.:	00001
		Soln. Date:	01/31/2009
		Soln. No.:	00005
		File Date:	01/31/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXD S3-0183
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0942

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:16S		
Control 1 EC	0.103%	08:17S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:17S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18S		
Control 2 EC	0.101%	08:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19S		
Control 3 EC	0.098%	08:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**  
 Last Name: SCHNEZLER      First Name: EDWARD      MI: J  
 Signature: *J.P.R.I. E. J. Schnezler #5515*      Badge No.: 5515  
 Date: 01/31/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00007	Calib. Date: 11/17/2008
Certification File No.:	00008	Calib. No.: 00002
Linearity File No.:	00009	Cert. Date: 11/17/2008
Solution File No.:	00014	Cert. No.: 00001
Sequential File No.:	00014	Lin. Date: 11/17/2008
		Lin. No.: 00001
		Soln. Date: 02/22/2009
		Soln. No.: 00006
		File Date: 02/22/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0928

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:21S		
Control 1 EC	0.102%	15:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:22S		
Control 2 EC	0.100%	15:23S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:24S		
Control 3 EC	0.100%	15:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:25S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

*TEMPERATURE PROBE SERIAL # DDWAP2-020 (RMD)*

**Changed By:**

Last Name: DEMLER

First Name: ROBERT

MI: M.

Signature: *Robert M. Demler*

Badge No.: 6073

Date: 02/22/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00007	Calib. Date: 11/17/2008
Certification File No.:	00008	Calib. No.: 00002
Linearity File No.:	00009	Cert. Date: 11/17/2008
Solution File No.:	00015	Cert. No.: 00001
Sequential File No.:	00015	Lin. Date: 11/17/2008
		Lin. No.: 00001
		Soln. Date: 03/23/2009
		Soln. No.: 00007
		File Date: 03/23/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0926

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:56S		
Control 1 EC	-.---%	07:57S	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	07:57S	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNEZLER

First Name: EDWARD

MI: J

Signature: TPRE J. Schnezler 5515

Badge No.: 5515

Date: 03/23/2009

Rubber Gasket  
 hose was not connected

ES

# Calibrating Unit New Standard Solution Report

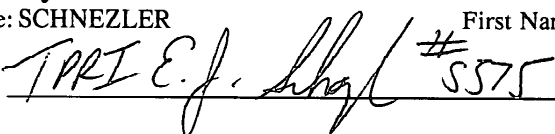
<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00007	Calib. Date: 11/17/2008
Certification File No.:	00008	Calib. No.: 00002
Linearity File No.:	00009	Cert. Date: 11/17/2008
Solution File No.:	00016	Cert. No.: 00001
Sequential File No.:	00016	Lin. Date: 11/17/2008
		Lin. No.: 00001
		Soln. Date: 03/23/2009
		Soln. No.: 00008
		File Date: 03/23/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0926

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:02S		
Control 1 EC	0.102%	09:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03S		
Control 2 EC	0.100%	09:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04S		
Control 3 EC	0.100%	09:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNEZLER	First Name: EDWARD	MI: J
Signature: <u></u>	Badge No.: 5515	Date: 03/23/2009

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00007	Calib. Date: 11/17/2008
Certification File No.:	00008	Calib. No.: 00002
Linearity File No.:	00009	Cert. Date: 11/17/2008
Solution File No.:	00017	Cert. No.: 00001
Sequential File No.:	00017	Lin. Date: 11/17/2008
		Lin. No.: 00001
		Soln. Date: 04/22/2009
		Soln. No.: 00009
		File Date: 04/22/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0938

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:32D		
Control 1 EC	0.101%	03:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:33D		
Control 2 EC	0.099%	03:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:34D		
Control 3 EC	0.099%	03:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	03:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:36D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: SCHNEZLER

First Name: EDWARD

MI: J

Signature: 

Badge No.: 5515

Date: 04/22/2009

# Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00018	Calib. No.: 00003
Certification File No.:	00019	Cert. No.: 00002
Linearity File No.:	00020	Lin. No.: 00002
Solution File No.:	00021	Soln. No.: 00010
Sequential File No.:	00021	File Date: 05/12/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0946

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:19D		
Control 1 EC	0.100%	14:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:20D		
Control 2 EC	0.099%	14:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:21D		
Control 3 EC	0.098%	14:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Serial Number Temp. Probe # DDWAP2-020

Changed By:

Last Name: ARROYO

First Name: MARCOS

MI: A.

Signature: Tpr. [Handwritten Signature] 6291

Badge No.: 6291

Date: 05/12/2009

# Calibrating Unit New Standard Solution Report

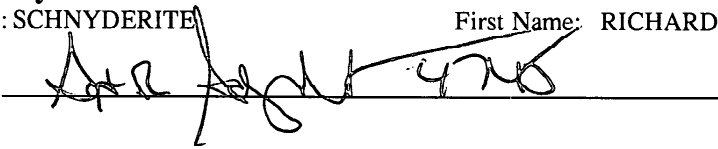
<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00018	Calib. Date: 05/12/2009
Certification File No.:	00019	Calib. No.: 00003
Linearity File No.:	00020	Cert. Date: 05/12/2009
Solution File No.:	00023	Cert. No.: 00002
Sequential File No.:	00023	Lin. Date: 05/12/2009
		Lin. No.: 00002
		Soln. Date: 07/09/2009
		Soln. No.: 00012
		File Date: 07/09/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0931

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:31D		
Control 1 EC	0.098%	13:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:33D		
Control 2 EC	0.097%	13:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:34D		
Control 3 EC	0.097%	13:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNYDERITE	First Name: RICHARD	MI: T
Signature: 	Badge No.: 4745	Date: 07/09/2009



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00027	Calib. Date: 10/16/2009
Certification File No.:	00028	Calib. No.: 00004
Linearity File No.:	00029	Cert. Date: 10/16/2009
Solution File No.:	00031	Cert. No.: 00003
Sequential File No.:	00031	Lin. Date: 10/16/2009
		Lin. No.: 00003
		Soln. Date: 10/23/2009
		Soln. No.: 00016
		File Date: 10/23/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0935

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:16D		
Control 1 EC	0.101%	10:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17D		
Control 2 EC	0.099%	10:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:19D		
Control 3 EC	0.098%	10:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SCHNEZLER

First Name: EDWARD

MI: J

Signature: *JPR. I E. f. Schnezler # 5575*

Badge No.: 5515

Date: 10/23/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00018	Calib. Date: 05/12/2009
Certification File No.:	00019	Calib. No.: 00003
Linearity File No.:	00020	Cert. Date: 05/12/2009
Solution File No.:	00024	Cert. No.: 00002
Sequential File No.:	00024	Lin. Date: 05/12/2009
		Lin. No.: 00002
		Soln. Date: 08/16/2009
		Soln. No.: 00013
		File Date: 08/16/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0936

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:29D		
Control 1 EC	0.101%	21:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	21:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:30D		
Control 2 EC	0.099%	21:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	21:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:31D		
Control 3 EC	0.098%	21:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: POWERS

First Name: MATTHEW

MI: N

Signature: \_\_\_\_\_

*Tpr. M. Powers #6472*

Badge No.: 6472

Date: 08/16/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0005
Location:	N.J.S.P. - NEWARK BAY		
Calibration File No.:	00018	Calib. Date:	05/12/2009
Certification File No.:	00019	Cert. Date:	05/12/2009
Linearity File No.:	00020	Lin. Date:	05/12/2009
Solution File No.:	00026	Soln. Date:	09/17/2009
Sequential File No.:	00026	File Date:	09/17/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWE S3-0168
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0948

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:19D		
Control 1 EC	0.101%	19:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:20D		
Control 2 EC	0.098%	19:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	19:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:22D		
Control 3 EC	0.098%	19:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: POWERS

First Name: MATTHEW

MI: N

Signature:

J.P.R. Powers # 6472

Badge No.: 6472

Date: 09/17/2009

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00027	Calib. Date: 10/16/2009
Certification File No.:	00028	Calib. No.: 00004
Linearity File No.:	00029	Cert. Date: 10/16/2009
Solution File No.:	00035	Cert. No.: 00003
Sequential File No.:	00035	Lin. Date: 10/16/2009
		Lin. No.: 00003
		Soln. Date: 12/29/2009
		Soln. No.: 00019
		File Date: 12/29/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWE S3-0168
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0943

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:45S		
Control 1 EC	0.101%	11:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:47S		
Control 2 EC	0.099%	11:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48S		
Control 3 EC	0.099%	11:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: POWERS

First Name: MATTHEW

MI: N

Signature:

*T.P.C. POWERS # 6472*

Badge No.: 6472

Date: 12/29/2009



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00027	Calib. Date: 10/16/2009
Certification File No.:	00028	Calib. No.: 00004
Linearity File No.:	00029	Cert. Date: 10/16/2009
Solution File No.:	00049	Cert. No.: 00003
Sequential File No.:	00049	Lin. Date: 10/16/2009
		Lin. No.: 00003
		Soln. Date: 02/25/2010
		Soln. No.: 00021
		File Date: 02/25/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDSC S3-0004
Solution Control Lot:	09D065	Expires: 04/22/2011
		Bottle No.: 0188

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:21S		
Control 1 EC	0.100%	07:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	07:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:23S		
Control 2 EC	0.098%	07:24S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	07:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:24S		
Control 3 EC	0.098%	07:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	07:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:26S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

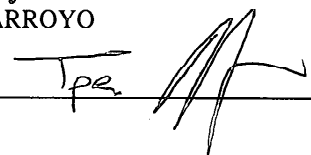
**Changed By:**

Last Name: ARROYO

First Name: MARCOS

MI: A.

Signature: \_\_\_\_\_



6291

Badge No.: 6291

Date: 02/25/2010

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWC-0005
Location:	N.J.S.P. - NEWARK BAY	
Calibration File No.:	00051	Calib. Date: 04/15/2010
Certification File No.:	00052	Calib. No.: 00005
Linearity File No.:	00053	Cert. Date: 04/15/2010
Solution File No.:	00054	Cert. No.: 00004
Sequential File No.:	00054	Lin. Date: 04/15/2010
		Lin. No.: 00004
		Soln. Date: 04/15/2010
		Soln. No.: 00023
		File Date: 04/15/2010

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDSC S3-0004
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0087

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:56D		
Control 1 EC	0.100%	16:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:58D		
Control 2 EC	0.098%	16:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:59D		
Control 3 EC	0.097%	17:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DD4N P2-397 (RMD)


**Changed By:**

Last Name: DEMLER

First Name: ROBERT

MI: M.

Signature: \_\_\_\_\_



Badge No.: 6073

Date: 04/15/2010