

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BIVALVE	
Calibration File No.:	00006	Calib. Date: 10/16/2008
Certification File No.:	00007	Calib. No.: 00002
Linearity File No.:	00008	Cert. Date: 10/16/2008
Solution File No.:	00009	Cert. No.: 00001
Sequential File No.:	00009	Lin. Date: 10/16/2008
		Lin. No.: 00001
		Soln. Date: 10/16/2008
		Soln. No.: 00002
		File Date: 10/16/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0265
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0769

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:47D		
Control 1 EC	0.102%	11:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:49D		
Control 2 EC	0.103%	11:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50D		
Control 3 EC	0.102%	11:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDUJ P2 - 062 *ans*

Changed By:

Last Name: STANKS

First Name: ADAM

MI: N

Signature: *TPR I Adam M. Stanks #5403*

Badge No.: 5403

Date: 10/16/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00010	Calib. Date: 03/11/2009
Certification File No.:	00011	Calib. No.: 00003
Linearity File No.:	00012	Cert. Date: 03/11/2009
Solution File No.:	00013	Cert. No.: 00002
Sequential File No.:	00013	Lin. Date: 03/11/2009
		Lin. No.: 00002
		Soln. Date: 03/11/2009
		Soln. No.: 00003
		File Date: 03/11/2009

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWF S3-0214
Control Solution %:	0.100%		Expires: 03/07/2010
Solution Control Lot:	08C051		Bottle No.: 0247

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:17S	15:170 25	
Control 1 EC	0.102%	14:17S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:17S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:18S		
Control 2 EC	0.100%	14:19S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:19S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:19S		
Control 3 EC	0.100%	14:20S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:20S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:21S	15:210 25	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: 00XK P2-4222

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *T.P. E.J. Sullivan #5103*

Badge No.: 5103

Date: 03/11/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00019	Calib. Date: 04/27/2009
Certification File No.:	00020	Calib. No.: 00006
Linearity File No.:	00021	Cert. Date: 04/27/2009
Solution File No.:	00022	Cert. No.: 00003
Sequential File No.:	00022	Lin. Date: 04/27/2009
		Lin. No.: 00003
		Soln. Date: 04/27/2009
		Soln. No.: 00005
		File Date: 04/27/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0214
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0761

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:30D		
Control 1 EC	0.100%	10:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:31D		
Control 2 EC	0.098%	10:32D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:32D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33D		
Control 3 EC	0.099%	10:33D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:33D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature probe Serial Number: DDX KPa-42235

Changed By:

Last Name: SULLIVAN	First Name: FRANCIS	MI: -
Signature: <u><i>Francis J Sullivan #5103</i></u>	Badge No.: 5103	Date: 04/27/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWC-0019
 Location: NJSP - BELLMAWR
 Calibration File No.: 00019 Calib. Date: 04/27/2009 Calib. No.: 00006
 Certification File No.: 00020 Cert. Date: 04/27/2009 Cert. No.: 00003
 Linearity File No.: 00021 Lin. Date: 04/27/2009 Lin. No.: 00003
 Solution File No.: 00025 Soln. Date: 05/21/2009 Soln. No.: 00006
 Sequential File No.: 00025 File Date: 05/21/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0214
 Control Solution %: 0.100% Expires: 03/07/2010
 Solution Control Lot: 08C051 Bottle No.: 0226

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:05D		
Control 1 EC	0.099%	10:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		
Control 2 EC	0.098%	10:07D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08D		
Control 3 EC	0.099%	10:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXP2-42225

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *Francis J Sullivan #5103*

Badge No.: 5103

Date: 05/21/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00019	Calib. Date: 04/27/2009
Certification File No.:	00020	Calib. No.: 00006
Linearity File No.:	00021	Cert. Date: 04/27/2009
Solution File No.:	00034	Cert. No.: 00003
Sequential File No.:	00034	Lin. Date: 04/27/2009
		Lin. No.: 00003
		Soln. Date: 06/24/2009
		Soln. No.: 00007
		File Date: 06/24/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0214
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0237

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:35D		
Control 1 EC	0.100%	06:36D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:36D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:37D		
Control 2 EC	0.099%	06:37D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:37D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:38D		
Control 3 EC	0.098%	06:39D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:39D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:39D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FONTANEZ

First Name: PEDRO

MI: P

Signature: _____

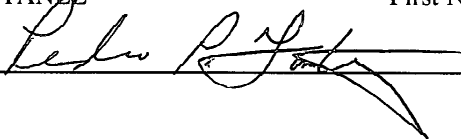

Badge No.: 4052

Date: 06/24/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00019	Calib. Date: 04/27/2009
Certification File No.:	00020	Calib. No.: 00006
Linearity File No.:	00021	Cert. Date: 04/27/2009
Solution File No.:	00040	Cert. No.: 00003
Sequential File No.:	00040	Lin. Date: 04/27/2009
		Lin. No.: 00003
		Soln. Date: 07/25/2009
		Soln. No.: 00008
		File Date: 07/25/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0214
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0244

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:38D		
Control 1 EC	0.101%	19:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:39D		
Control 2 EC	0.099%	19:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:41D		
Control 3 EC	0.099%	19:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	19:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DIAZ	First Name: RICARDO	MI: -
Signature: <u>TPR. R. [Signature] #6783</u>	Badge No.: 6783	Date: 07/25/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0019
Location:	NJSP - BELLMAWR		
Calibration File No.:	00019	Calib. Date:	04/27/2009
Certification File No.:	00020	Cert. No.:	00006
Linearity File No.:	00021	Calib. No.:	00003
Solution File No.:	00048	Cert. Date:	04/27/2009
Sequential File No.:	00048	Lin. Date:	04/27/2009
		Soln. Date:	08/25/2009
		File Date:	08/25/2009
		Soln. No.:	00009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	4
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0768

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:23D		
Control 1 EC	0.100%	16:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:24D		
Control 2 EC	0.099%	16:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:26D		
Control 3 EC	0.099%	16:26D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FONTANEZ

First Name: PEDRO

MI: P

Signature: _____

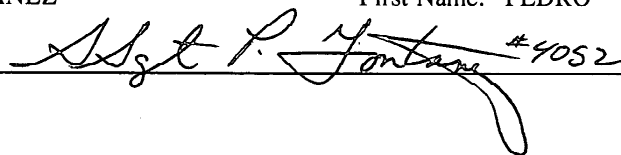

Sgt P. Fontanez #4052

Badge No.: 4052

Date: 08/25/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0019
Location:	NJSP - BELLMAWR	Calib. Date:	04/27/2009
Calibration File No.:	00019	Calib. No.:	00006
Certification File No.:	00020	Cert. Date:	04/27/2009
Linearity File No.:	00021	Lin. Date:	04/27/2009
Solution File No.:	00051	Soln. Date:	09/06/2009
Sequential File No.:	00051	File Date:	09/06/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	4
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0753

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:06D		
Control 1 EC	----%	03:06D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	----%	03:06D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	----%	--:--		
Control 2 EC	----%	--:--	N/A	
Control 2 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		
Control 3 EC	----%	--:--	N/A	
Control 3 IR	----%	--:--	N/A	
Ambient Air Blank	----%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: TOMPKINS	First Name: ROBERT	MI: S
Signature: <u><i>Sgt. A. Tompkins #5157</i></u>	Badge No.: 5107	Date: 09/06/2009

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWC-0019
 Location: NJSP - BELLMAWR
 Calibration File No.: 00019 Calib. Date: 04/27/2009 Calib. No.: 00006
 Certification File No.: 00020 Cert. Date: 04/27/2009 Cert. No.: 00003
 Linearity File No.: 00021 Lin. Date: 04/27/2009 Lin. No.: 00003
 Solution File No.: 00052 Soln. Date: 09/08/2009 Soln. No.: 00011
 Sequential File No.: 00052 File Date: 09/08/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: 4
 Control Solution %: 0.100% Expires: 03/07/2010
 Solution Control Lot: 08C051 Bottle No.: 0772

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:06D		
Control 1 EC	0.100%	01:07D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	01:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:07D		
Control 2 EC	0.098%	01:08D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:09D		
Control 3 EC	0.099%	01:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:10D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FONTANEZ

First Name: PEDRO

MI: P

Signature: _____

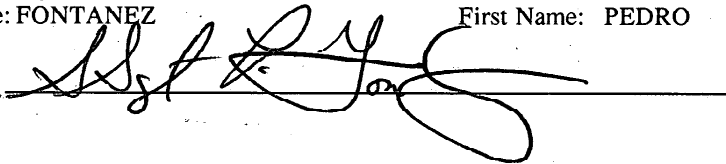

Badge No.: 4052

Date: 09/08/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0019
Location:	NJSP - BELLMAWR		
Calibration File No.:	00059	Calib. Date:	10/08/2009
Certification File No.:	00060	Calib. No.:	00007
Linearity File No.:	00061	Cert. Date:	10/08/2009
Solution File No.:	00062	Cert. No.:	00004
Sequential File No.:	00062	Lin. Date:	10/08/2009
		Lin. No.:	00004
		Soln. Date:	10/08/2009
		Soln. No.:	00012
		File Date:	10/08/2009
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWF S3-0214
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0771

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:17D		
Control 1 EC	0.101%	10:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:19D		
Control 2 EC	0.099%	10:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 3 EC	0.099%	10:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXKPa-42235

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *Tr. I J Sullivan #5103*

Badge No.: 5103

Date: 10/08/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00059	Calib. Date: 10/08/2009
Certification File No.:	00060	Calib. No.: 00007
Linearity File No.:	00061	Cert. Date: 10/08/2009
Solution File No.:	00071	Cert. No.: 00004
Sequential File No.:	00071	Lin. Date: 10/08/2009
		Lin. No.: 00004
		Soln. Date: 11/10/2009
		Soln. No.: 00013
		File Date: 11/10/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0214
Solution Control Lot:	08C051	Expires: 03/07/2010
		Bottle No.: 0764

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:22S		
Control 1 EC	0.100%	14:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:23S		
Control 2 EC	0.098%	14:24S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:25S		
Control 3 EC	0.098%	14:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:26S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXKP2-42235

Changed By:

Last Name: SULLIVAN	First Name: FRANCIS	MI: -
Signature: <u><i>Tr D Sullivan #5103</i></u>		Badge No.: 5103
		Date: 11/10/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00059	Calib. Date: 10/08/2009
Certification File No.:	00060	Calib. No.: 00007
Linearity File No.:	00061	Cert. Date: 10/08/2009
Solution File No.:	00078	Cert. No.: 00004
Sequential File No.:	00078	Lin. Date: 10/08/2009
		Lin. No.: 00004
		Soln. Date: 11/28/2009
		Soln. No.: 00014
		File Date: 11/28/2009

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWF S3-0214
Control Solution %: 0.100%		Expires: 03/07/2010
Solution Control Lot: 08C051		Bottle No.: 0755

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:04S		
Control 1 EC	0.100%	09:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05S		
Control 2 EC	0.098%	09:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:06S		
Control 3 EC	0.098%	09:07S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:08S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ENGELHARD

First Name: DAVID

MI: J

Signature:  #6722

Badgc No.: 6722

Date: 11/28/2009

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0019
Location:	NJSP - BELLMAWR		
Calibration File No.:	00059	Calib. Date:	10/08/2009
Certification File No.:	00060	Calib. No.:	00007
Linearity File No.:	00061	Cert. Date:	10/08/2009
Solution File No.:	00085	Lin. Date:	10/08/2009
Sequential File No.:	00085	Lin. No.:	00004
		Soln. Date:	01/02/2010
		Soln. No.:	00015
		File Date:	01/02/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWF S3-0214
Solution Control Lot:	08C051	Expires:	03/07/2010
		Bottle No.:	0228

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:22S		
Control 1 EC	0.103%	02:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	02:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:24S		
Control 2 EC	0.099%	02:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	02:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:25S		
Control 3 EC	0.099%	02:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FONTANEZ

First Name: PEDRO

MI: P

Signature: _____



Badge No.: 4052

Date: 01/02/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: NJSP - BELLMAWR
Calibration File No.: 00059
Certification File No.: 00060
Linearity File No.: 00061
Solution File No.: 00093
Sequential File No.: 00093

Serial No.: ARWC-0019

Calib. Date: 10/08/2009
Cert. Date: 10/08/2009
Lin. Date: 10/08/2009
Soln. Date: 02/02/2010
File Date: 02/02/2010

Calib. No.: 00007
Cert. No.: 00004
Lin. No.: 00004
Soln. No.: 00016

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 08C051

Model No.: CU-34

Serial No.: DDWF S3-0264
Expires: 03/07/2010
Bottle No.: 0014

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:38S		
Control 1 EC	0.101%	14:38S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:39S		
Control 2 EC	0.098%	14:40S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41S		
Control 3 EC	0.099%	14:41S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:42S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXA P2-04735

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *Tr. J. Sullivan #5103*

Badge No.: 5103

Date: 02/02/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLEMAWR	
Calibration File No.:	00059	Calib. Date: 10/08/2009
Certification File No.:	00060	Calib. No.: 00007
Linearity File No.:	00061	Cert. Date: 10/08/2009
Solution File No.:	00108	Cert. No.: 00004
Sequential File No.:	00108	Lin. Date: 10/08/2009
		Lin. No.: 00004
		Soln. Date: 02/25/2010
		Soln. No.: 00017
		File Date: 02/25/2010

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWF S3-0264
Control Solution %:	0.100%		Expires: 07/01/2011
Solution Control Lot:	09G067		Bottle No.: 0844

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:22S		
Control 1 EC	0.099%	06:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:24S		
Control 2 EC	0.098%	06:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	06:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:25S		
Control 3 EC	0.100%	06:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	06:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:27S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: APPLGATE

First Name: PAUL

MI: J

Signature: _____



Badge No.: 6774

Date: 02/25/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00059	Calib. Date: 10/08/2009
Certification File No.:	00060	Calib. No.: 00007
Linearity File No.:	00061	Cert. Date: 10/08/2009
Solution File No.:	00124	Cert. No.: 00004
Sequential File No.:	00124	Lin. Date: 10/08/2009
		Lin. No.: 00004
		Soln. Date: 03/09/2010
		Soln. No.: 00018
		File Date: 03/09/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0264
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0829

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:11S		
Control 1 EC	0.101%	00:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:12S		
Control 2 EC	0.099%	00:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	00:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:14S		
Control 3 EC	0.099%	00:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CASTELLANO

First Name: VINCENT

MI: J

Signature: 

Badge No.: 5035

Date: 03/09/2010

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C
Location: NJSP - BELLMAWR
Calibration File No.: 00059
Certification File No.: 00060
Linearity File No.: 00061
Solution File No.: 00132
Sequential File No.: 00132

Serial No.: ARWC-0019

Calib. Date: 10/08/2009 Calib. No.: 00007
Cert. Date: 10/08/2009 Cert. No.: 00004
Lin. Date: 10/08/2009 Lin. No.: 00004
Soln. Date: 03/16/2010 Soln. No.: 00019
File Date: 03/16/2010

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 09G067

Model No.: CU-34
Serial No.: DDWF S3-0264
Expires: 07/01/2011
Bottle No.: 0833

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:55S <i>12:55D</i>		
Control 1 EC	0.100%	11:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 2 EC	0.099%	11:57S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58S		
Control 3 EC	0.100%	11:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59S <i>12:59D</i>		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DOXAPF: 04725

Changed By:

Last Name: SULLIVAN

First Name: FRANCIS

MI: -

Signature: *Tr. ID Sullivan #5103*

Badge No.: 5103

Date: 03/16/2010

Calibrating Unit New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00143	Calib. Date: 03/31/2010
Certification File No.:	00144	Calib. No.: 00008
Linearity File No.:	00145	Cert. Date: 03/31/2010
Solution File No.:	00159	Cert. No.: 00005
Sequential File No.:	00159	Lin. Date: 03/31/2010
		Lin. No.: 00005
		Soln. Date: 04/16/2010
		Soln. No.: 00021
		File Date: 04/16/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0264
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0830

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:46D		
Control 1 EC	0.100%	04:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:47D		
Control 2 EC	0.097%	04:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	04:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:49D		
Control 3 EC	0.098%	04:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:50D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LAWRENCE	First Name: TROOPER	MI: -
Signature: <u></u>	Badge No.: 6582	Date: 04/16/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00143	Calib. Date: 03/31/2010
Certification File No.:	00144	Calib. No.: 00008
Linearity File No.:	00145	Cert. Date: 03/31/2010
Solution File No.:	00186	Cert. No.: 00005
Sequential File No.:	00186	Lin. Date: 03/31/2010
		Lin. No.: 00005
		Soln. Date: 05/10/2010
		Soln. No.: 00023
		File Date: 05/10/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0264
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0837

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:41D		
Control 1 EC	0.100%	10:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		
Control 2 EC	0.099%	10:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:44D		
Control 3 EC	0.098%	10:45D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:46D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXAP2-047js

Changed By:

Last Name: SULLIVAN	First Name: FRANCIS	MI: -
Signature: <u><i>Tr I J Sullivan #5103</i></u>	Badge No.: 5103	Date: 05/10/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWC-0019
Location:	NJSP - BELLMAWR	Calib. Date:	03/31/2010
Calibration File No.:	00143	Calib. No.:	00008
Certification File No.:	00144	Cert. Date:	03/31/2010
Linearity File No.:	00145	Lin. Date:	03/31/2010
Solution File No.:	00199	Soln. Date:	06/05/2010
Sequential File No.:	00199	File Date:	06/05/2010
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWF S3-0264
Solution Control Lot:	09G067	Expires:	07/01/2011
		Bottle No.:	0846

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:38D		
Control 1 EC	0.101%	18:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:39D		
Control 2 EC	0.100%	18:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:41D		
Control 3 EC	0.099%	18:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:42D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUTEPOW

First Name: ADAM

MI: M

Signature: _____

[Handwritten Signature]
#6646

Badge No.: 6646

Date: 06/05/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00143	Calib. Date: 03/31/2010
Certification File No.:	00144	Calib. No.: 00008
Linearity File No.:	00145	Cert. Date: 03/31/2010
Solution File No.:	00219	Cert. No.: 00005
Sequential File No.:	00219	Lin. Date: 03/31/2010
		Lin. No.: 00005
		Soln. Date: 06/27/2010
		Soln. No.: 00025
		File Date: 06/27/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0264
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0836

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:16D		
Control 1 EC	0.099%	03:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	03:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:18D		
Control 2 EC	0.098%	03:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:19D		
Control 3 EC	0.098%	03:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: JACOBS

First Name: WILLIAM

MI: S

Signature: _____

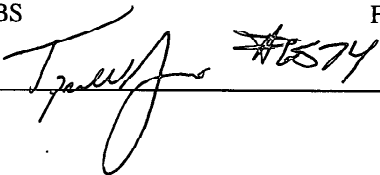

Badge No.: 6574

Date: 06/27/2010

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWC-0019
Location:	NJSP - BELLMAWR	
Calibration File No.:	00143	Calib. Date: 03/31/2010
Certification File No.:	00144	Calib. No.: 00008
Linearity File No.:	00145	Cert. Date: 03/31/2010
Solution File No.:	00231	Cert. No.: 00005
Sequential File No.:	00231	Lin. Date: 03/31/2010
		Lin. No.: 00005
		Soln. Date: 07/25/2010
		Soln. No.: 00026
		File Date: 07/25/2010
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWF S3-0264
Solution Control Lot:	09G067	Expires: 07/01/2011
		Bottle No.: 0071

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:31D		
Control 1 EC	0.101%	23:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:32D		
Control 2 EC	0.099%	23:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:33D		
Control 3 EC	0.099%	23:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:35D		

▣ All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CONWAY

First Name: MICHAEL

MI: J

Signature: *Trn. M. Conway # 7103*

Badge No.: 7103

Date: 07/25/2010