

**Dräger**safety

**Alcotest<sup>®</sup> 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.


Certification Date:

06.17.2005

SERIAL NUMBER:

ARWE-0038

**Draeger Safety Diagnostics, Inc.**  
Durango, CO

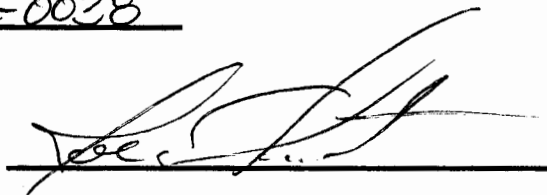

**Dräger**safety

**Alcotest<sup>®</sup> 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


03-11-08

SERIAL NUMBER:

ARWE-0038

**Draeger Safety Diagnostics, Inc.**  
Durango, CO

  
\_\_\_\_\_



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

**Recreated on  
03/18/2008**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDSC 53 - 0010

Certification Date

Technician

Re-Certification Due Date

FEB. 25/2008

TG

FEB. 25/2009

## Dräger safety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUNP2-439

02-25-08

02-25-09

Probe Value

102

Draeger Safety Diagnostics, Inc.  
Technical Service Department



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0021

Certification Date

Technician

Re-Certification Due Date

02.13.08

*[Signature]*

02.13.09



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0022

Certification Date

Technician

Re-Certification Due Date

02.13.08

*[Signature]*

02.13.09



**Dräger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0024

Certification Date

02-13-08

Technician

[Signature]

Re-Certification Due Date

02-13-09

**Dräger**safety

**ALCOTEST® 7110 TEMPERATURE PROBE**

## CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA P2-038

Certification date:

02-12-08

Next Certification due:


02-12-09

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

[Signature]



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34  
 Model: MARK IIA  
 Other: \_\_\_\_\_

Serial Number:

DDWF 53-0245

Certification Date


Technician

Re-Certification Due Date

JUNE 6, 2005

DB

JUNE 6, 2006



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWF53-0245

Certification Date

Technician

Re-Certification Due Date

3/16/07

mk

3/16/08

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXAP2-128

02/23/2007


02/23/2008

Probe Value

104

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

CS



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDMK 53-0007

Certification Date

MAR 09 2006

Technician

DB

Re-Certification Due Date

MAR 09 2007



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDMK53-0007

Certification Date

Technician

Re-Certification Due Date

FEB 19 2007

*[Signature]*

FEB 19 2009



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRK53-0011

Certification Date


Technician

Re-Certification Due Date

FEB 19 2007

*[Signature]*

FEB 19 2009



Draeger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DRK 53-0011

Certification Date


MAR 09 2006

Technician

DB

Re-Certification Due Date

MAR 09 2007



Draeger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK II A
- Other: \_\_\_\_\_

Serial Number:

DDWJ 53-0334

Certification Date

FAR 0 9 2006

Technician

DB

Re-Certification Due Date

FAR 0 9 2007



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWTS3 - 0334

Certification Date

01/03/2007

Technician

CRS

Re-Certification Due Date

01/03/2008

## Dräger safety

### ALCOTEST<sup>®</sup> 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest<sup>®</sup> 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest<sup>®</sup> 7110.

Serial Number Temp. Probe

DDMBP1 - 0004

Certification date:

11/27/2006

Next Certification due:


11/27/2007

Probe Value

103

Draeger Safety Diagnostics, Inc.  
Technical Service Department

CRS



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST<sup>®</sup> CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXD 53-0181

Certification Date

Technician

Re-Certification Due Date

APR 13 2006

DB

APR 13 2007

**Dräger**safety

**ALCOTEST® 7110 TEMPERATURE PROBE**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below,

must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-037

Certification date:

06-09-2005

Next Certification due:

06-09-2006

Probe Value

101

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department



**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXAP2-013

04/12/2006

04/12/2007

Probe Value

105

Draeger Safety Diagnostics, Inc.  
Technical Service Department

Cent Dely

**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDMBP1-0004

11/27/2006


11/27/2007

Probe Value

103

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

CS



**Dräger**safety

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXD 53-0181

Certification Date

Technician

Re-Certification Due Date

APR 13 2006

DB

APR 13 2007

**Dräger**safety

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDMSPI-0004

Certification date:

03/09/2006

Next Certification due:

03/09/2007

Probe Value

103

Draeger Safety Diagnostics, Inc.  
Technical Service Department

Autry

# Dräger safety

Ertco-Hart Digital Temperature Measuring System

## REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature  
verification Serial Number: AH41 303176

Digital Units Serial Number: A 23730

Probe Serial Number: 583983

Certification Date: 03-14-2005

Next Certification Due: 03-14-2006

At 34.00 °C digital unit displays 33.99 °C

Draeger Safety Diagnostics, Inc. Technician: 

## Ertco-Hart Digital Temperature Measuring System

### REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: HH41 301316 / HH41 303176 / MERCURY THERMOMETER

Digital Units Serial Number: A23727


Probe Serial Number: 5B3982

Certification Date: 02-12-2008

Next Certification Due: 02-12-2009

At 34.00 °C digital unit displays 34.06 °C

Draeger Safety Diagnostics, Inc. Technician: *AE*



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDRK53-0021

Certification Date


Technician

Re-Certification Due Date

02-03-2009

*[Signature]*

02-03-2010



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDRK53-0022

Certification Date


Technician

Re-Certification Due Date

02/03/2009

*[Signature]*

02/03/2010



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0024

Certification Date

Technician

Re-Certification Due Date

02/03/2009

JR

02/03/2010

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWAP2-038

02/03/2009


02/03/2010

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Services Department

JR



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDWFS3-0249

Certification Date

02-09-09

Technician

[Signature]

Re-Certification Due Date

02-09-10

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-028

Certification date:

02/10/2009

Next Certification due:

02/10/2010

Probe Value

104

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

[Signature]



# Calibration complies with ISO 9001 ISO/IEC 17025 AND ANSI/NCSL Z540-1



Calibration  
Certificate No. 1750.01

Cert. No.: 4000-2023730

## Traceable® Certificate of Calibration for Digital Thermometer

### Instrument Identification:

Model: 61220-601      S/N: 80614942      Manufacturer: Control Company

### Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC191 Digital Thermometer	A79341 72310620/72310747	7/01/09	4000-1923693
Temperature Calibration Bath TC179 Digital Thermometer	A45240 22136727	5/16/09	4000-1882244
Temperature Probe Thermistor Module	149 A17118	3/06/09 11/15/08	A82225037-3 A7831032
Temperature Calibration Bath TC218	A73332		

### Certificate Information:

Technician: 68      Procedure: CAL-06      Cal Date: 11/04/08      Cal Due: 11/04/10  
Test Conditions: 23.5°C      44.0 %RH      1019 mBar

### Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±uc	TUR
°C		N.A.		0.001	0.001	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.004	24.999	Y	24.954	25.054	0.013	3.8:1
°C		N.A.		60.001	59.998	Y	59.951	60.051	0.018	2.8:1
°C		N.A.		100.001	99.999	Y	99.951	100.051	0.013	3.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein are the property of Control Company.

*Wallace Berry*  
Wallace Berry, Technical Manager

### Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

### Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

**CONTROL COMPANY** 4455 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-0180S-AQ-HOU.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



**Drägersafety**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0023

Certification Date

1-18-10

Technician

mm

Re-Certification Due Date

1-18-11

**Drägersafety**

**ALCOTEST® 7110 TEMPERATURE PROBE**

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWA P2-111

Certification date:

1/19/10

Next Certification due:


1/19/11

Probe Value

105

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

2M



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0021

Certification Date

Technician

Re-Certification Due Date

4-14-10

MM

4-14-11



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0022

Certification Date


Technician

Re-Certification Due Date

2/3/10

DM

2/3/11



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRKS3-0024

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-038

Certification date:

2-3-10

Next Certification due:

2-3-11

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

gmm